



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Pacesetter Alpacas/Dennis Pace
5546 W Plymouth Church Rd
Beloit WI 53511 USA

09/03/15

Test No: 913802


Animal and Sample Description

Animal Name: Dolly
Breed: Alpaca(Suri)
Sex: Female
Color: Black

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/23/15
Age: 06/04/13

Laboratory Data

Mean Fiber Diameter: 25.0 microns
Standard Deviation: 5.2 microns
Coefficient of Variation: 21.0 %
Fibers Greater Than 30 microns: 10.1 %

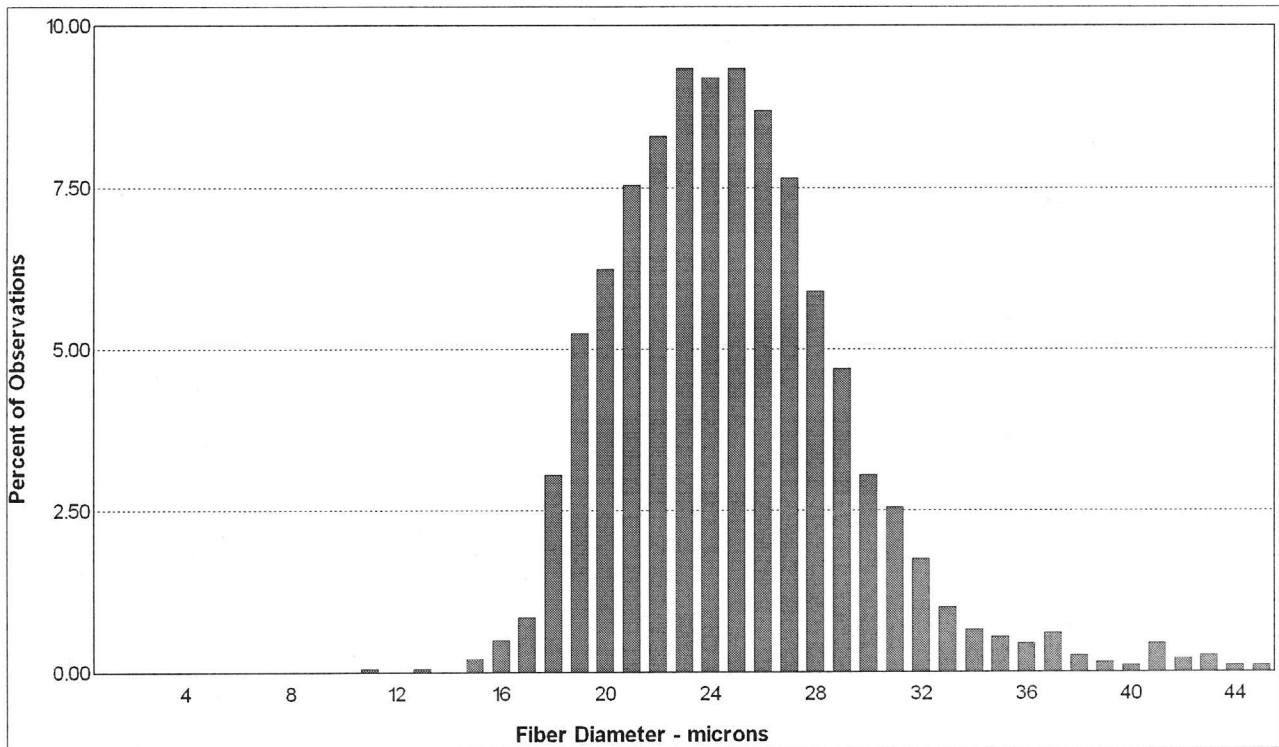

This Test Performed According to I.W.T.O Method 12