



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Morgan's Fortunato Farm/Ben & Gina Morgan
122 Fortunato Lane
Waverly WV 26184 USA

07/30/12

Test No: 437582


Animal and Sample Description

Animal Name: Abraham
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 036308817
Sample Location: Side (R)
Sample Date: 04/26/12
Age: XXXXX

Laboratory Data

Mean Fiber Diameter:	16.9 microns	Spin Fineness:	17.0 microns
Standard Deviation:	4.1 microns	Mean Curvature (deg/mm):	43.9
Coefficient of Variation:	24.5 %	SD Curvature (deg/mm):	25.3
Fibers Greater Than 30 microns:	0.3 %	Comfort Factor:	99.7 %
Medullated Fibers:	7.5 %		

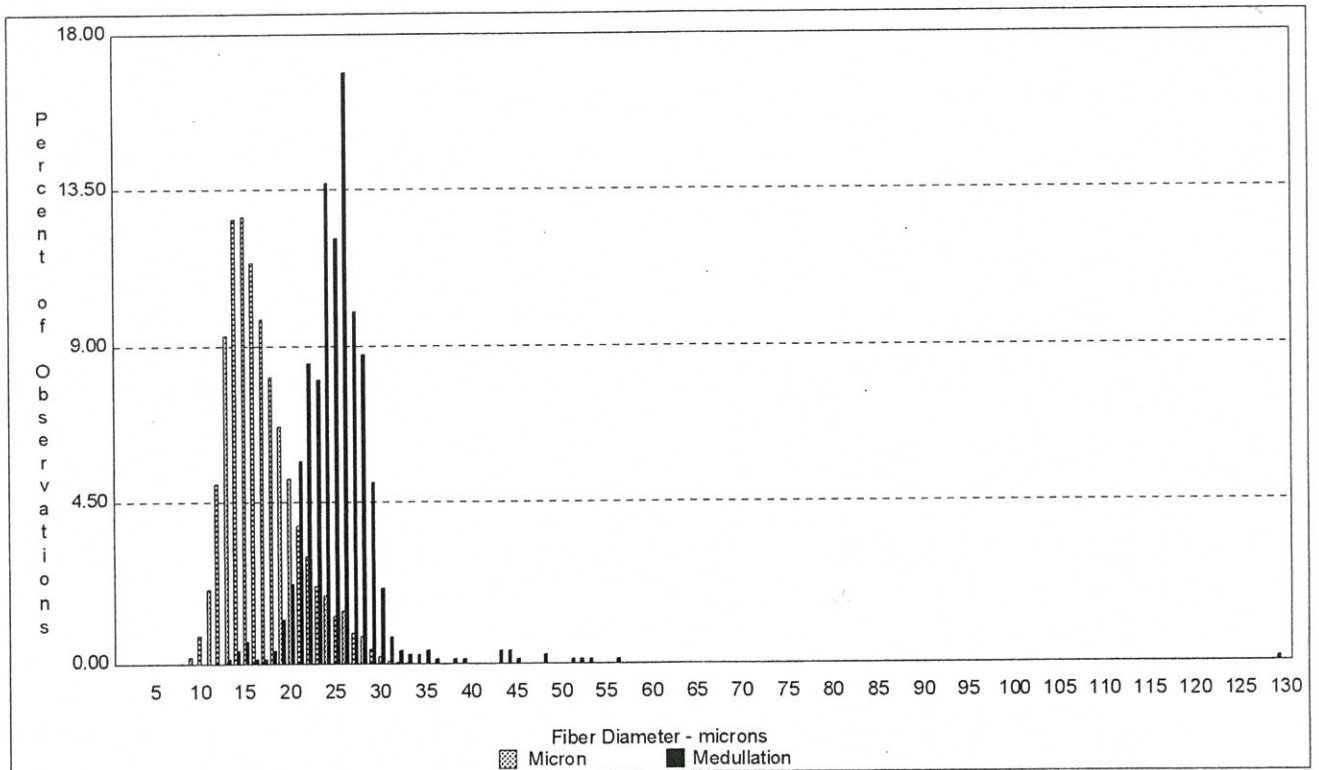

This Test Performed According to I.W.T.O Method 47