



## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Sirolan Laserscan Micron Test Report

MapleView Alpacas/Edwin G Pierrot  
8462 Christmiller Rd  
Otto NY 14766 USA

07/28/14

Test No: 487208


#### Animal and Sample Description

**Animal Name:** MapleVeiv's Ella Jay  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Lt Fawn

**Animal ID:** 32468465  
**Sample Location:** Side  
**Sample Date:** 05/25/14  
**Age:** 05/01/13

#### Laboratory Data

**Mean Fiber Diameter:** 18.6 microns  
**Standard Deviation:** 3.6 microns  
**Coefficient of Variation:** 19.4 %  
**Fibers Greater Than 30 microns:** 1.4 %

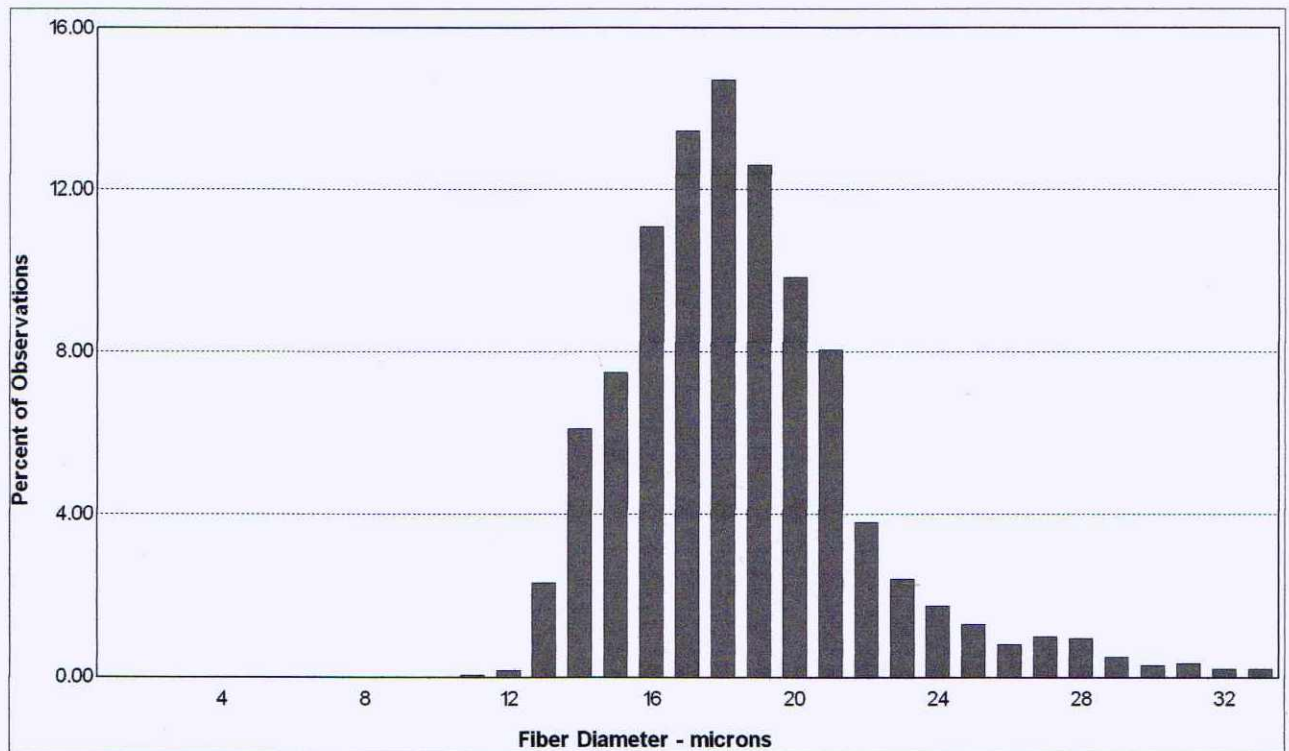

This Test Performed According to I.W.T.O Method 12