



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Green Acres Alpacas/David & Sherry Bishop
11087 Bazile Rd
Glen Allen VA 23059 USA

Date: 05/08/15

Test No: 500391


Animal and Sample Description

Animal Name: Jocelyn
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Silver Grey

Animal ID: XXXXX
Sample Location: Mid Side
Sample Date: 04/05/15
Age: 04/14/13

Laboratory Data

Mean Fiber Diameter:	26.9 microns	Fibers Greater Than 30 microns:	17.8 %
Standard Deviation:	9.3 microns	Comfort Factor:	82.2 %
Coefficient of Variation:	34.4 %	Mean Curvature:	31.4 deg/mm
Spin Fineness:	29.9 microns	SD Curvature:	19.3 deg/mm

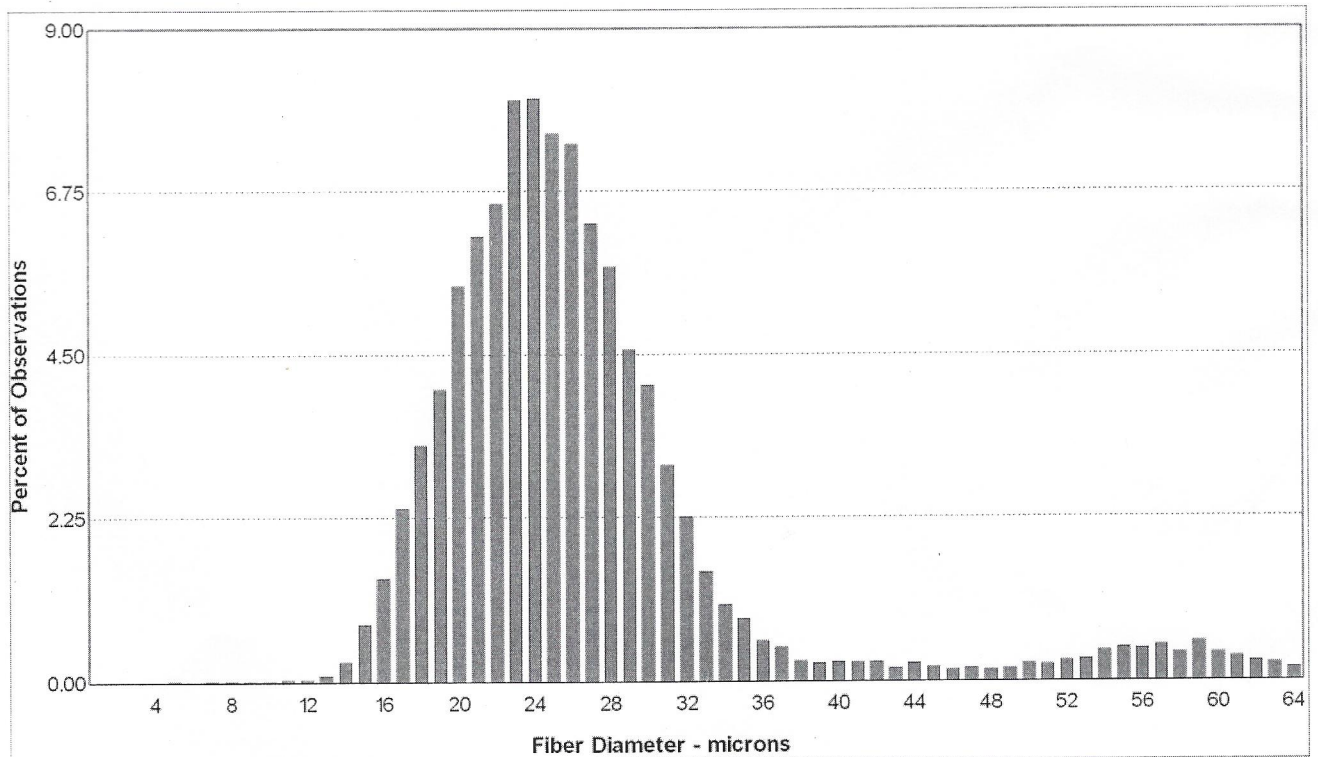

This Test Performed According to I.W.T.O Method 47