



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Mile High Alpacas/Sharon Loner
12818 N Woodland Trail
Parker CO 80138 U.S.A.

06/08/09

Test No: 351083


Animal and Sample Description

Animal Name: Mile High Peerless Bay
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Fawn

Animal ID: 30661226
Sample Location: Side
Sample Date: 05/19/09
Age: 04/09/07

Laboratory Data

Mean Fiber Diameter: 20.7 microns
Standard Deviation: 4.8 microns
Coefficient of Variation: 23.4 %
Fibers Greater Than 30 microns: 3.0 %

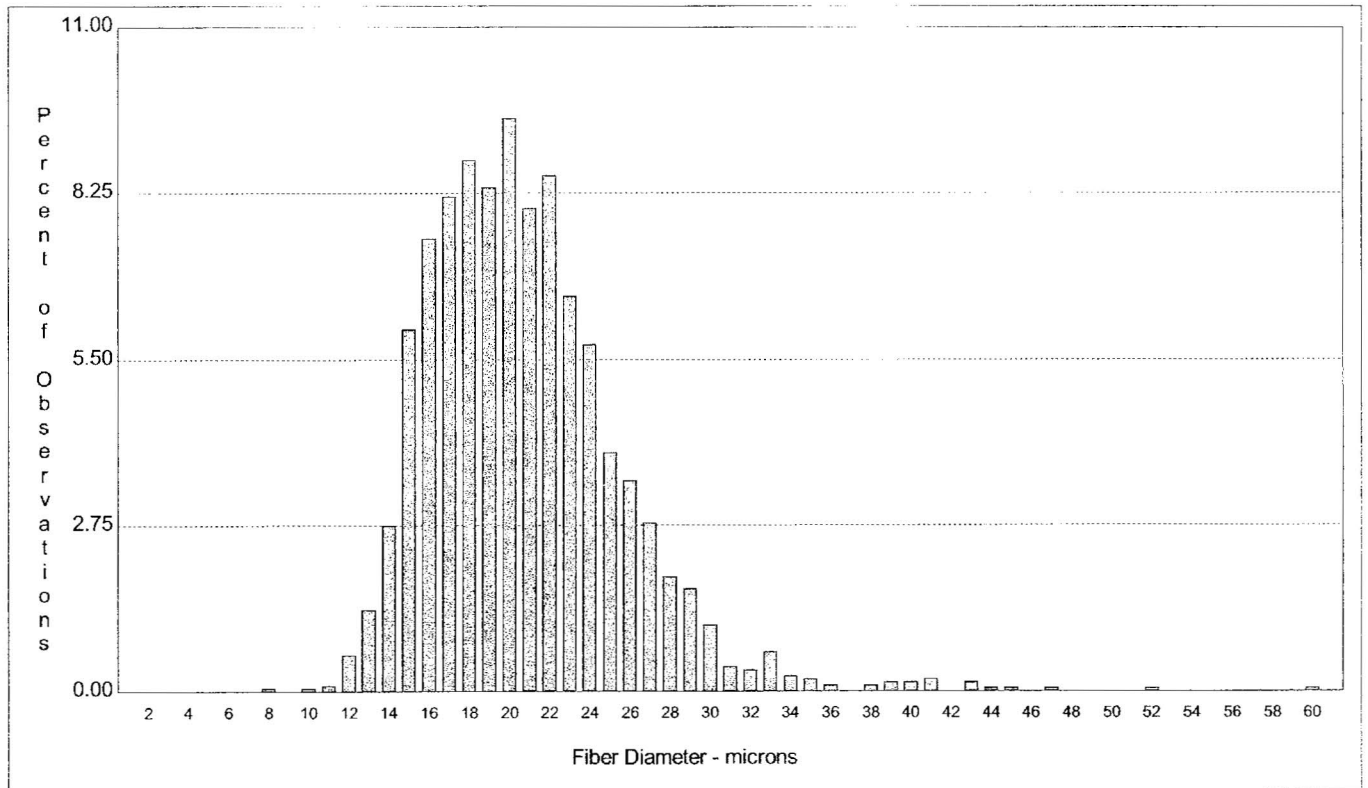

This Test Performed According to I.W.T.O Method 12