



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Starshire Ranch/June Aploks  
8300 Robbins Rd  
Ellensburg WA 98926 USA

08/15/17

Test No: 949919


### Animal and Sample Description

**Animal Name:** Tarik  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** XXXXX

**Animal ID:** 35256632  
**Sample Location:** Side  
**Sample Date:** 05/13/17  
**Age:** 05/20/15

### Laboratory Data

**Mean Fiber Diameter:** 16.3 microns  
**Standard Deviation:** 2.9 microns  
**Coefficient of Variation:** 17.6 %  
**Fibers Greater Than 30 microns:** 0.3 %

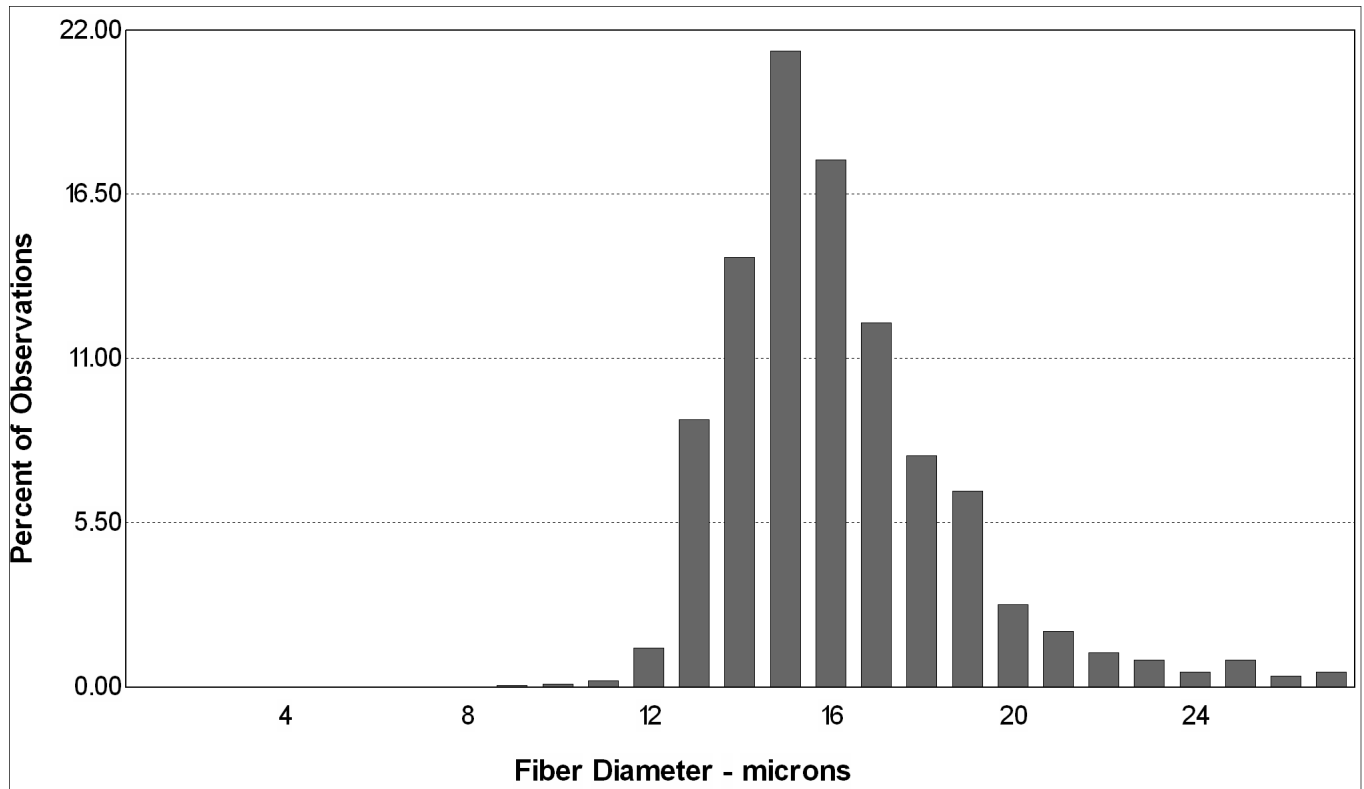

This Test Performed According to I.W.T.O Method 12